

# Airtraq<sup>sp</sup>

## VIDEO LARYNGOSCOPE FOR DOUBLE LUMEN ENDOTRACHEAL TUBES

US Patent No 6,843,769

### INSTRUCTIONS FOR USE

REF: A071; A871

#### INTENDED USE AND DESCRIPTION

Airtraq SP DL is a video laryngoscope to facilitate intubation when using double lumen endobronchial tubes (DLT). It allows visualization of the airway during intubation. It minimizes hyper extension of the neck and permits intubating from virtually any position. ET Tube is loaded into the lateral channel of the device and when advanced it is guided towards the glottis of the patient.

It is a SINGLE USE medical device provided clean and ready to use.

To perform its purpose Airtraq SP must have attached to its proximal end, either

- its eyecup or
- the WiFi Camera (Ref A-390) offered by the manufacturer, attached after removing its eyecup, or
- an Endoscopic camera attached to the eyecup.

#### SIZES AND SPECIFICATIONS

##### Double Lumen Tubes: A-071

For use with double lumen tubes sizes 28-41 Fr.

Any style of DLT (right-sided or left-sided, Carina hooked or not hooked) can be used.

Minimum patient mouth opening: 18 mm

Maximum insertion portion width: 33.8 mm.

Working Length: 117.3 mm.

Field of View: Vertical 32 degrees; Horizontal 27 degrees

Direction of View: Vertical 112 degrees; Horizontal 12 degrees

#### USE INSIDE OF THE MRI ENVIRONMENT

This medical device was determined to be MR conditional according to the terminology specified by ASTM Standard Practice for Marking Medical Devices and Other Items for Safety in the Magnetic Resonance Environment.

The device can be used in the MRI environment according to the following conditions:

- Static magnetic field of 3-Tesla or less
- Spatial gradient magnetic field of 720-Gauss/cm or less

**IMPORTANT NOTE:** The device is intended for use inside of the MRI environment (e.g., in the MR system room). It will not be utilized directly inside of the MR system (e.g., inside of the bore of the scanner), during its operation (i.e., scanning). As such, the assessment of magnetic field interactions for the device specifically involved evaluations of translational attraction in relation to exposure to a 3-Tesla MR system, only.

#### TECHNIQUE FOR USING THE AIRTRAQ SP DL

##### I. PREPARATION & TEST

- Press orange switch located below the battery cover to Turn On the light.
- After 30 seconds check that the light is steady. If so, anti-fog system is fully activated.

**NOTE: If light automatically turns off, the unit has become defective and must not be used.**


- Remove the stylet from inside DLT.
- Check DLT cuffs and fully deflate both.
- Lubricate (preferably using water soluble lubricant, not spray) the lower 1/3 of the DLT and place it into the lateral channel of the Airtraq SP DL.

#### ORIENTATION OF THE DLT IN THE AIRTRAQ SP DL GUIDING CHANNEL.

- Load the DLT and orient the deviated tip of the DLT so it points towards the light of the Airtraq SP DL. If the DLT tube is a right side stylet, then rotate the DLT 180 degrees until the deviated tip of the of the right DL tube is pointing towards the light of the Airtraq SP DL.
- If the DLT has a carina hook, the hook should point toward the open side of the Airtraq SP DL guiding channel.
- Lubricate the DLT and place it into the lateral channel of the Airtraq SP DL without contacting the lens.
- Align the tip of the DLT with the end of the guide channel.

#### II. AIRTRAQ SP DL PLACEMENT (Fig. 1)


- Insert the Airtraq SP DL along midline of the patient's mouth. Take care to avoid pushing the tongue inside the oropharynx.
- Advance the Airtraq SP DL through the oropharynx keeping it in the midline.
- Before it reaches the vertical plane, begin looking to identify airway structures.
- Continue insertion until the epiglottis is identified. Place the tip of the Airtraq SP DL in the vallecula. Alternatively, the tip can be placed under the epiglottis, lifting it out of the way.
- Gently lift up the Airtraq SP DL to expose the vocal cords.

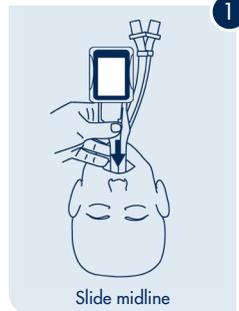

- Do not insert too deep

#### III. DLT INSERTION (Fig. 2)


- **Align the vocal cords in the center of the visual field** by gently moving the tip of the Airtraq SP DL as needed.
- Gently advance the DLT while in the guiding channel. STOP advancing when the DLT proximal cuff has just passed through the vocal cords. Do not insert further. This places the DLT at approximately the midpoint of the trachea. Check insertion depth.
- Inflate the DLT cuff as normal and check for proper positioning.

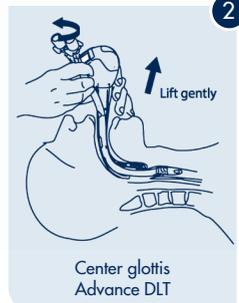

- Lift gently
- Twist Airtraq to center vocal cords
- Corkscrew ETT

#### IV. AIRTRAQ SP DL REMOVAL (Fig. 3)

- Separate the DLT from the Airtraq SP DL by pulling it laterally from the guiding channel, while holding the DLT in position.
- Check final insertion depth and location in the bronchi pursuant to hospital standard protocol, e.g. stethoscope or fiberoptic bronchoscope).
- Remove the Airtraq SP DL from the patient's airway following the midline.

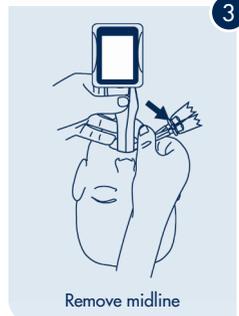

## WARNINGS AND PRECAUTIONS

- This product should only be used by personnel trained in insertion of Double Lumen Endobronchial tubes (DLT).
- Do not sterilize.
- Do not incinerate unless batteries have been removed.
- Do not submerge in liquids.
- Use only with non-flammable anesthetics.
- Do not put pressure on the teeth with this device.
- Do not force the Airtraq SP DL into the upper airway.

## USAGE TIPS

1. Initial experience should be gained in non-difficult airways.
2. Lubricate DLT generously (preferably using water soluble lubricants, not spray) and check that cuffs are fully deflated).
3. Insert the Airtraq SP DL, avoiding the tongue, and slide it softly and slowly.
4. Keep the Airtraq SP DL in the mouth's midline.
5. Look before the Airtraq SP DL gets to the vertical plane.
6. Do not insert too deep. If structures (arytenoids, epiglottis, etc.) are not clearly recognized or tube cannot be inserted, withdraw the Airtraq SP DL slightly.
7. Once the tip is located at the epiglottis, either at the vallecula (Macintosh style), or under the epiglottis (Miller style), gently lift up the Airtraq SP DL (do not tilt or use a lever action).
8. Advance the DLT slowly. If needed rotate DLT inside the channel.

## BATTERY CHARACTERISTICS

Each Airtraq SP DL is equipped with two AAA batteries in serial connection that provide a voltage of 3 volts. The batteries provide power to the LED light and to the anti-fog system when the switch is turned on. They should not be replaced.

## STORAGE, TRANSPORT, SHELF LIFE AND SERVICE LIFE

The Airtraq SP DL should not be used, stored or transported at temperatures below -5°C/23°F or over 55°C/131°F. The relative humidity must not exceed 95%. The air pressure must not exceed 500 to 1060 hPa.

Airtraq SP DL shelf life is limited to the expiration date.

Airtraq SP DL service life is limited to 40 accumulative minutes, 5 minutes before its end; the Airtraq SP DL will start blinking for 2 seconds every 20 seconds. Once maximum operating time is reached the Airtraq SP DL will blink continuously until battery is depleted.

## DISPOSAL

To dispose the Airtraq SP DL once it has been used:

- Separate the eyecup from the main body by pulling it up.
- Remove the battery cover by pulling it away from the main body (pull away from the small notches).
- Remove the batteries from the Airtraq SP DL and place them in an appropriate battery recycling container (dispose of them according to established recycling policies). The batteries are classified as non hazardous waste material and comply with European Directive WEEE. However, the manufacturer recommends separating them from standard trash.
- Discard the Airtraq SP DL as any other potentially contaminated waste.

## MANUFACTURER'S WARRANTY

The manufacturer warrants the Airtraq SP DL against faulty materials or manufacturing defects for only one use or until the expiration date, whichever comes first, provided that the Airtraq SP DL is used in accordance with the procedures set forth in these instructions. This Warranty is applicable only if the device is purchased from an authorized distributor.

This device has not been designed to be cleaned or sterilized. Use beyond this recommendation may generate serious consequences in the product's performance and will void the Airtraq SP's warranty. The manufacturer disclaims all other warranties,

whether expressed or implied, including, without limitation, the warranties of merchantability or fitness for a particular use.

## USER ASSISTANCE INFORMATION

Instructions for use are available online at

<https://www.airtraq.com/IFU>

Visit [www.airtraq.com](http://www.airtraq.com) for further advice on using this device. Any serious incident that occurs in relation to this device should be reported to the manufacturer and the competent Health Authority in which the user and/or patient is established. For communication with manufacturer, please email [user.assistance@airtraq.com](mailto:user.assistance@airtraq.com), or:

1. Contact directly with Manufacturer at its address or by phone:  
USA & Canada: +1877-624-7929  
EU & Other: +34944804690
2. Contact Manufacturer's Representative for your area (details below) or
3. Contact your Local Distributor

### PRODOL MEDITEC LIMITED

1/F, 4/F, Block C,  
No. 18, 7th Science Ave.,  
Zhuhai, Guangdong,  
519085 P.R. China

### EC REP & EUROPE

**PRODOL MEDITEC S.A.**  
Muelle Tomás Olavarri 5, 3°  
48930 Las Arenas. SPAIN

### UK Responsible Person:

Advena  
Pure Offices, Plato Close,  
Tachbrook Park,  
Warwick, CV34 6WE, UK

### USA & Canada Representative:

D. A. Daniel  
2414 Lawton Ln.  
Rowlet, TX 75089, USA

Airtraq is a registered trademark.



Rx Only



[www.airtraq.com/ifu](http://www.airtraq.com/ifu)



## GLOSSARY OF SYMBOLS

SYMBOL	SYMBOL MEANING	SYMBOL	SYMBOL MEANING	SYMBOL	SYMBOL MEANING
	Reference Number		Number of Units		Legal Manufacturer
	Batch code		Manufacturing Date		Use-By date
	Authorized representative in the European Community		Importer		Medical device
	Fragile, handle with care		Consult instructions for use		Do not re-use
	Temperature limit.		Humidity limitation		Atmospheric Pressure Limitation
	Not Made with Natural Rubber Latex		Keep Dry / Protect from moisture		Federal (USA) law restricts the use of this device to sale by or on the order of a physician
	CE Mark, European Conformity		EAC Mark, Eurasian Conformity		UKCA Mark, UK Conformity Assessment
	This side up		Do not use if package is damaged		Distributor
	Separate collection for waste of electrical and electronic equipment		Type BF applied part		Australian sponsor
	Magnetic resonance conditional		Box/packaging recyclable		